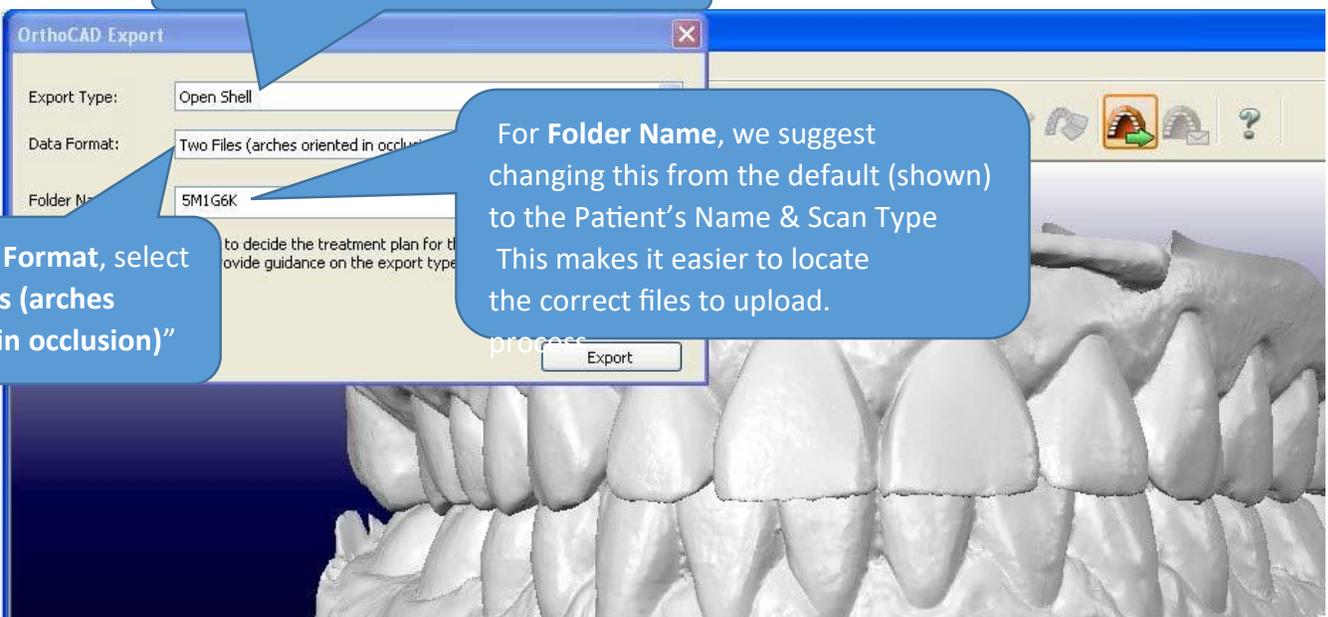# BI DESIGN
DIGITAL DENTAL CERAMICS

1-780-885-0016

How to Export Scans as .STL Files from an iTero Scanner

1. Open your web browser and Login to your MyAlignTech account

2. Search for the patient's scans you wish to export.

3. Select **Export (OrthoCAD 3.5 or higher).** This will download the image into OrthoCAD and open dialogue for completing the STL export.

For the **Export Type**, select **Open Shell**

For **Folder Name**, we suggest changing this from the default (shown) to the Patient's Name & Scan Type This makes it easier to locate the correct files to upload.

For **Data Format**, select "Two Files (arches oriented in occlusion)"

4. Click on the **Export** button and then click **Yes**. You should now be able to view the folder and .STL files. *To view the .STL files you can install the **iTero Viewer**. Click **Support** for installation instructions, or other viewer.*

5. Your scans are now saved as .STL files on your computer in the folder you specified. Be sure to make a note of where the files were saved. These files will need to be located when you are ready to Drop Box them to Bi Design Ceramics.

   We recommend creating a Case File folder to store both the Scans and the Rx Sheet to make it easier to locate during the upload process.